





Installation instructions



312/DS-039/5

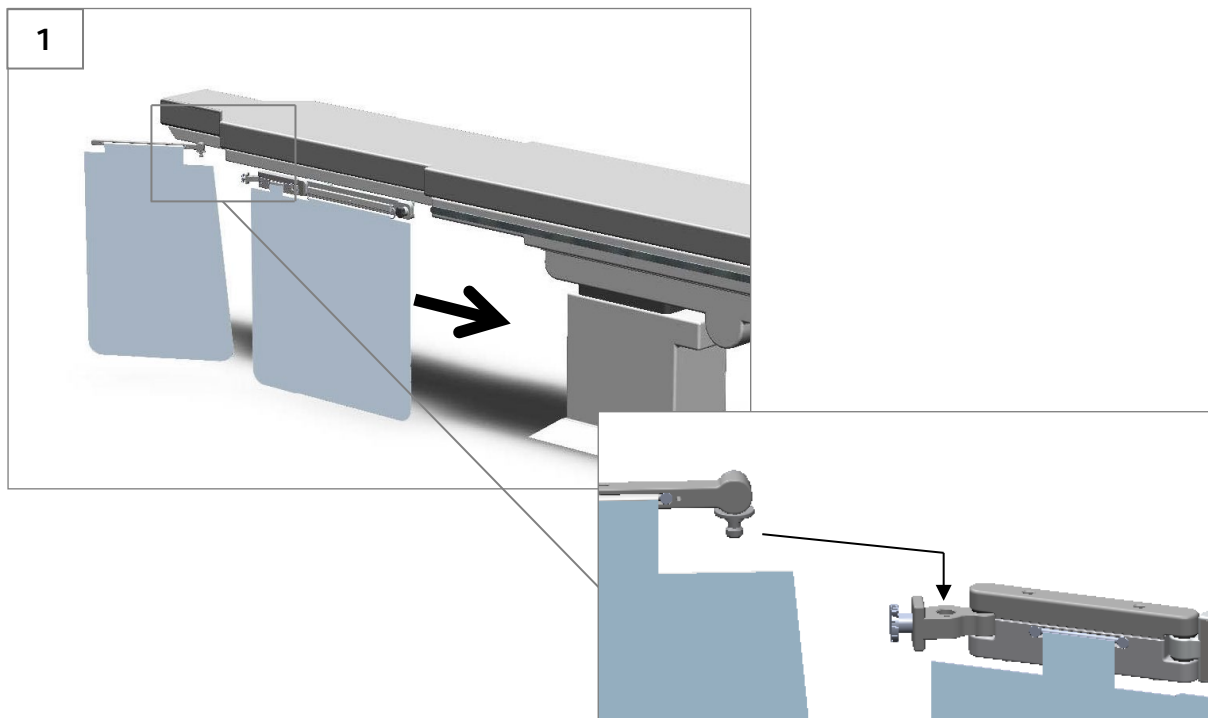

Kenex (Electro-Medical) Ltd, Unit 17, RO24 Greenway, Harlow Business Park, Harlow, Essex CM19 5QB, England
T: +44 (0)1279 417241 F: +44 (0)1279 443749 E: kenex@kenex.co.uk www.kenex.co.uk

Doc: INS 312_DS-039_5 issue 7 (05/03/2024)

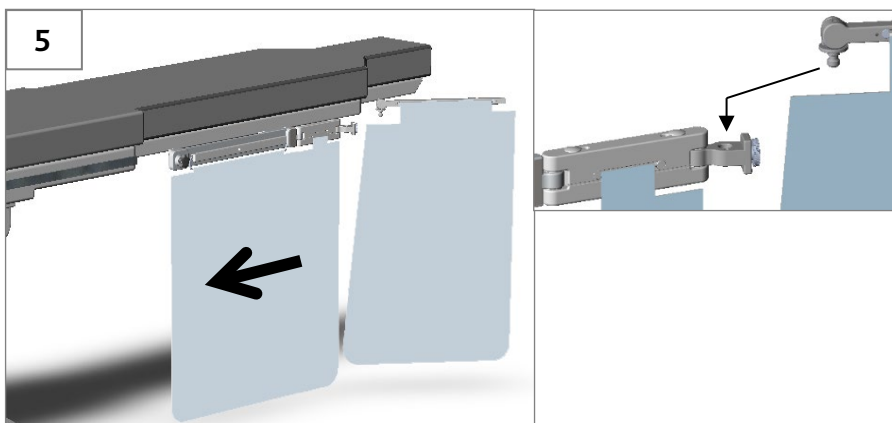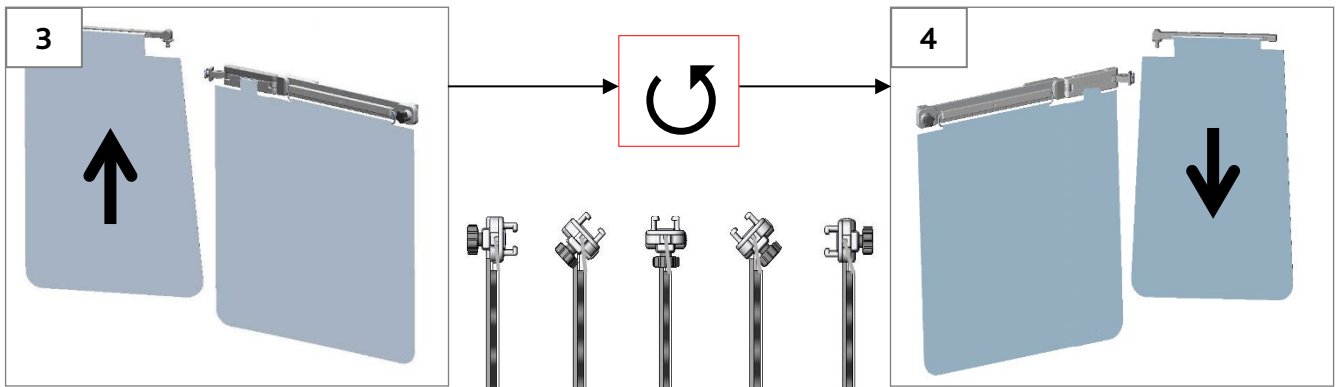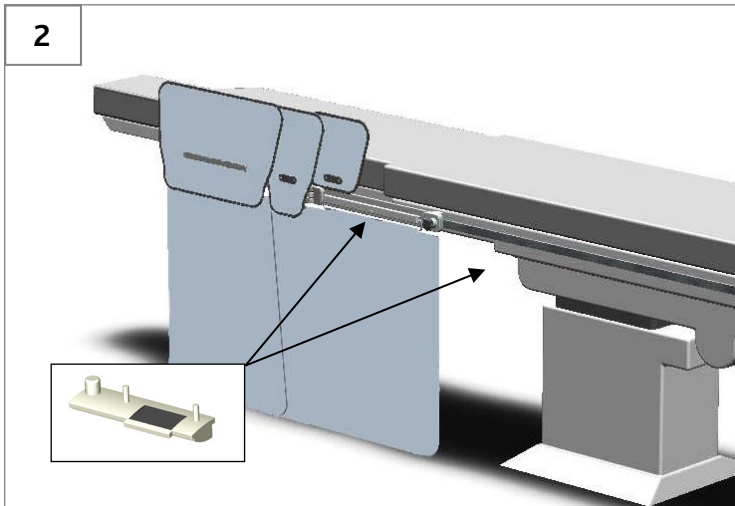

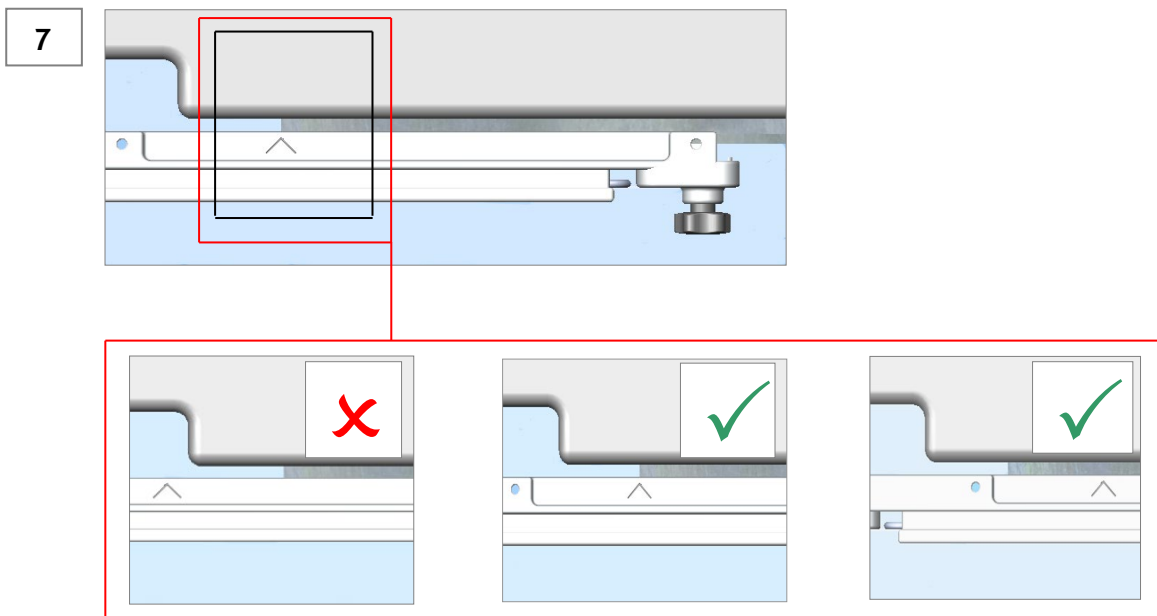
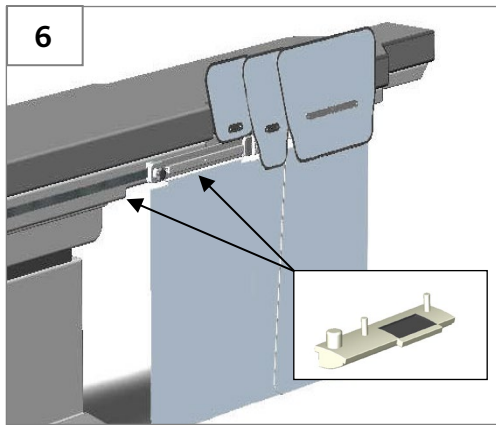


Optional top shields

- ❶ 312/DS/3.32/3
- ❷ 312/DS/3.30
- ❸ 312/DS/3.41



Recycling

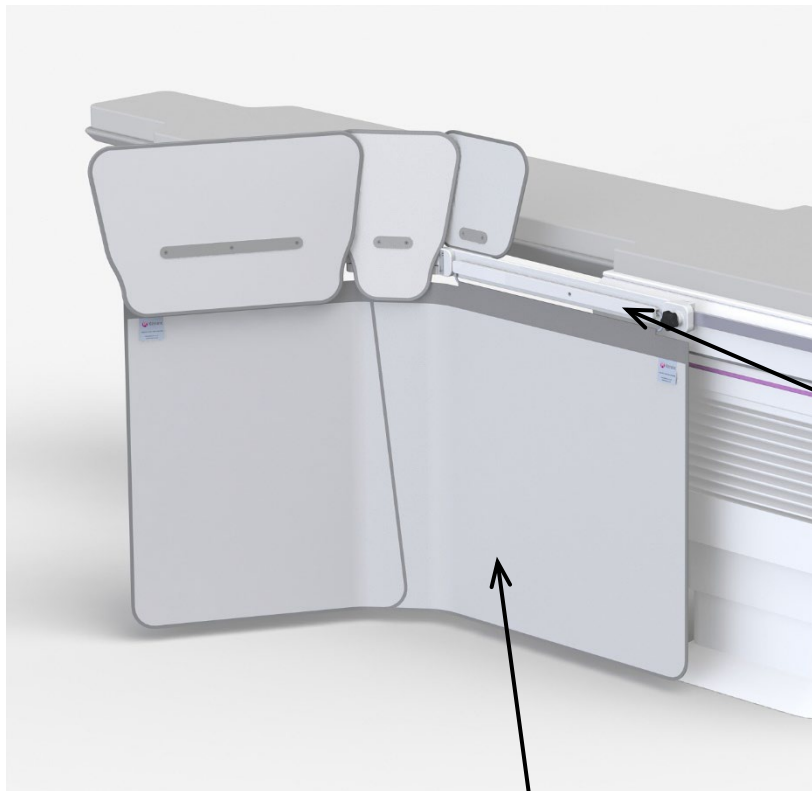

Aluminium (Al)

PVC + Pb = Classified as non hazardous waste
European Waste Catalogue (EWC) code 12 01 99

Cleaning



All devices should be cleaned using a mild soap solution or a regular hand dishwashing product. Do not spray on – wipe on with a damp cloth.



Kenex (Electro-Medical) Ltd, Unit 17, RO24 Greenway, Harlow Business Park, Harlow, Essex CM19 5QB, England
T: +44 (0)1279 417241 F: +44 (0)1279 443749 E: kenex@kenex.co.uk www.kenex.co.uk

Doc: INS 312_DS-039_5 issue 7 (05/03/2024)